


# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

JUL 06 2010

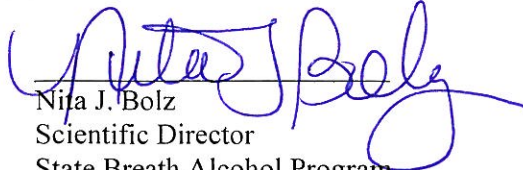
Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130309 ✓
Name		PATRICK NELSON	ID# 4389 ✓ Date 7/1/10 ✓
A	Agency	AST	Phone # 373-8337
Instrument Location		MSW	
Alco S/N		X172971 ✓	Target Value .083 ✓ High Pressure 1250
B	Alco Test Values	1st Alco .084 ✓	2nd Alco .084 ✓
Signature			
(OVER)			

BMS  
7/12/10

I, Nita J. Bolz, after being first duly sworn, depose and state as follows: (Do Not write in the area below)

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 27<sup>th</sup> day of July, 2010.

 (Notary Seal Stamp)

Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office



# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130309

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130309

JULY 01, 2010

OPERATOR'S NAME:  
NELSON PATRICK S  
OPERATOR'S NUMBER: 4389  
SUBJECT'S LAST NAME:  
VERIFICATION OF  
SUBJECT'S FIRST NAME/MI :  
CALIBRATION  
O.L. #: 123456  
DEPT/AGENCY: PLH0  
CASE/REPORT: 12-34567  
TEST TYPE: V  
ALCO TARGET VALUE: .083  
ALCO S/N: X172971

--- BREATH ANALYSIS ---

.083 ADJUSTED FOR 29.86 in  
ALCO TARGET .082 00:39  
BLANK TEST .000 00:40  
INTERNAL STANDARD VERIFIED 00:40  
ALCO TV 29.86 in .084 00:40  
BLANK TEST .000 00:41  
SUBJECT SAMPLE .000 00:42  
BLANK TEST .000 00:42  
ALCO TV 29.86 in .084 00:43  
BLANK TEST .000 00:44

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130309

JULY 01, 2010  
TIME 00:44

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 02/20/01  
HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 41c  
BAROMETER: 29.86 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

PRINTER TEST

! " # \$ % ' ( ) \* + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G  
H I J K L M N O P Q R S T U V W X Y Z [ \ ] ^ \_ ` a b c d e f g h i j k l m n o  
p q r s t u v w x y z { | } ~